**1. PERFORMANCE**

- 1) Measuring range : 0.004-1.0 %  
     Number of pump stroke     1 (100ml)
- 2) Sampling time           : 1 minute/1 pump stroke  
   3) Detectable limit       : 0.0005 % (5ppm)  
   4) Shelf life             : 1 year (Necessary to store in refrigerated conditions ; 0 ~ 10 °C)  
   5) Operating temperature   : 0 ~ 40 °C  
   6) Temperature compensation : Necessary (See "TEMPERATURE CORRECTION TABLE")  
   7) Reading               : Concentration chart method  
   8) Colour change        : Yellow → Pink

**2. RELATIVE STANDARD DEVIATION**

RSD-low : 10 %   RSD-mid. : 5 %   RSD-high : 5 %

**3. CHEMICAL REACTION**

By reacting with Hydroxylamine hydrochloride, Hydrogen chloride is liberated and PH indicator discoloured.

$$\text{CH}_3\text{CHO} + \text{NH}_2\text{OH} \cdot \text{HCl} \rightarrow \text{HCl} + \text{CH}_3\text{CH} = \text{NOH} + \text{H}_2\text{O}$$
**4. CALIBRATION OF THE TUBE**

GAS CHROMATOGRAPHY

**5. INTERFERENCE AND CROSS SENSITIVITY**

Substance	Interference	ppm	Coexistence
Acetone FIG.1	Similar stain is produced	1400	Higher readings are given.
Acrolein FIG.2	〃	35	〃
Methyl ethyl ketone	〃	900	〃
Methyl isobutyl ketone	〃	2900	〃

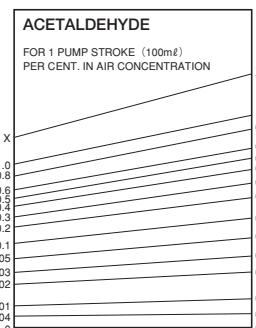




Chart Readings (%)	Corrected Concentration (%)				
	0 °C (32°F)	10 °C (50°F)	20 °C (68°F)	30 °C (86°F)	40 °C (104°F)
1.0	1.0	1.6	1.0	0.50	0.30
0.8	0.8	1.3	0.8	0.40	0.20
0.6	0.6	1.05	0.6	0.30	0.16
0.5	0.5	1.45	0.5	0.25	0.14
0.4	0.4	1.3	0.4	0.20	0.13
0.3	0.3	1.2	0.65	0.3	0.11
0.2	0.2	0.95	0.45	0.2	0.08
0.1	0.1	0.6	0.2	0.1	0.05
0.05	0.05	0.25	0.09	0.05	0.03
0.03	0.03	0.08	0.05	0.03	0.02
0.02	0.02	0.05	0.02	0.015	0.007
0.01	0.01	0.02	0.015	0.01	0.004
0.004					